

PRAFO (Pressure Relief Ankle Foot Orthosis)

General Description:

A PRAFO is a device that is worn on the calf and foot similar to a boot and is often used for patients that spend the majority of their time in bed.

One reason for its use is to prevent bedsores or ulcers from developing on the back of the heel. A bedsore or decubitus ulcer is caused by constant pressure on the back of the heel that can occur when lying in one position for prolonged periods of time. A PRAFO creates an air space around the back of the heel, alleviating pressure and preventing heel ulcers.

A second reason for the use of a PRAFO is to position the foot. While lying down, a person usually has the foot pointed downward at the ankle and this is called plantar flexion. This is not a problem for short intervals, but muscle tightness develops when the foot is not ranged upward at the ankle (dorsiflexed). The result is that deformities can develop called contractures.


When a plantar flexion contracture develops, normal range of motion is lost and the person will not be able to flex the foot upwards. If it becomes severe enough, the person will only be able to stand on the forefoot with the heel off of the ground.

Application:

1. With most patients, range the foot into dorsiflexion to at least a neutral position. This means to bring the foot upward so that the bottom of the foot is perpendicular to the lower leg (see figure 1). This is the normal procedure. If your healthcare provider does not want the foot to be ranged in this manner, other instructions will be provided.
2. Place the lower leg in the device with the foot in full contact with the footplate and the calf in even contact with the calf section (see figure 2). The PRAFO can also be applied with the knee bent, pushing the foot downward and back fully within the device.
3. Secure the straps over the foot and then secure the top calf strap (see figures 3 and 4).

| | | | | |
|--|--|---|--|--|
| <p>Arlington Heights 617 E. Golf Road, Suite 108 Arlington Heights, IL 60005 847-437-3929</p> | <p>Bannockburn 2101 Waukegan Road, Suite 104 Bannockburn, IL 60015 847-444-0690</p> | <p>Lincoln Park/Chicago 2551 N. Clark St., Suite 200 Chicago, IL 60614 773-472-3663</p> | <p>Rush/Chicago 1725 W. Harrison St. Suite 220 Chicago, IL 60612 312-942-2011</p> | <p>UIC/Chicago 1740 W. Taylor St. Room C100 Chicago, IL 60612 312-996-6450</p> |
| <p>Hickory Hills 8641 W. 95th St. Hickory Hills, IL 60457 708-599-8336</p> | <p>Naperville 1551 Bond St., Suite 111 Naperville, IL 60563 630-637-4638</p> | <p>Oakbrook Terrace 1S376 Summit Ave., Ct. E Oakbrook Terrace, IL 60181 630-424-0392</p> | <p>Oak Park 401 Harrison Street Oak Park, IL 60304 708-383-2257</p> | <p>Schererville 6629 W. Lincoln Hwy. (Rt. 30), Suite 1 PO Box 507 Schererville, IN 46375 219-864-9501</p> |

4. Finally, make sure that the heel is fully suspended in the air and that it is not in direct contact with the device (see figure 5). If it is, the device may not have been put on properly. If you are not able to do this correctly, contact your practitioner.
5. This device has an outrigger attached to the back of the calf section to prevent the leg from rolling to one side or the other. If instructed to use it by your healthcare provider, simply rotate it out in the direction the leg has a tendency to turn toward (see figure 6).

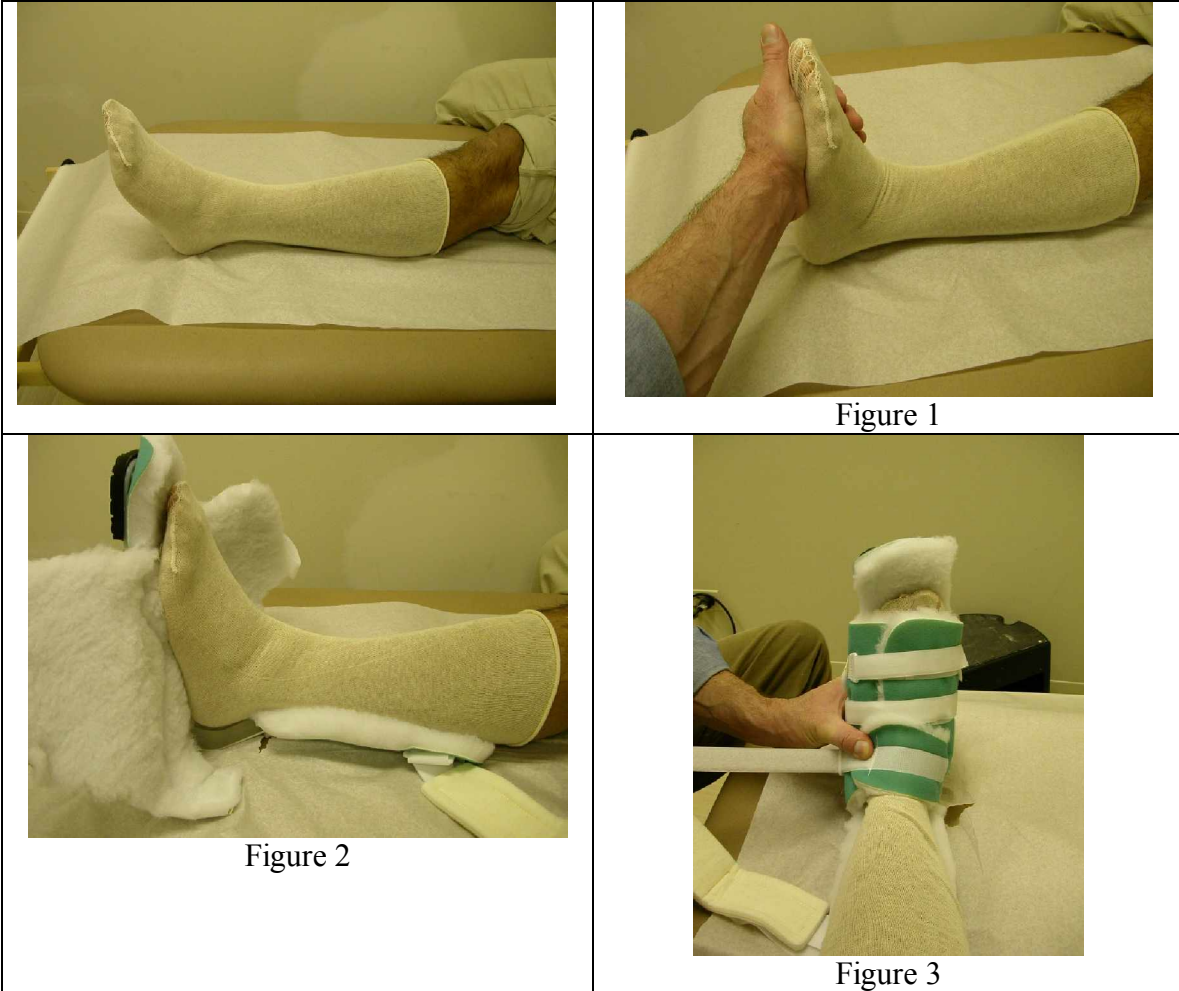

Arlington Heights
617 E. Golf Road, Suite 108
Arlington Heights, IL 60005
847-437-3929

Bannockburn
2101 Waukegan Road,
Suite 104
Bannockburn, IL 60015
847-444-0690

Lincoln Park/Chicago
2551 N. Clark St., Suite 200
Chicago, IL 60614
773-472-3663

Rush/Chicago
1725 W. Harrison St.
Suite 220
Chicago, IL 60612
312-942-2011

UIC/Chicago
1740 W. Taylor St.
Room C100
Chicago, IL 60612
312-996-6450

Hickory Hills
8641 W. 95th St.
Hickory Hills, IL 60457
708-599-8336

Naperville
1551 Bond St., Suite 111
Naperville, IL 60563
630-637-4638

Oakbrook Terrace
1S376 Summit Ave., Ct. E
Oakbrook Terrace, IL 60181
630-424-0392

Oak Park
401 Harrison Street
Oak Park, IL 60304
708-383-2257

Schererville
6629 W. Lincoln Hwy.
(Rt. 30), Suite 1
PO Box 507
Schererville, IN 46375
219-864-9501



Figure 4



Figure 5



Figure 6

Care and maintenance:

The liner can be removed and washed at a temperature below 150 degrees and dried using a cool low setting. When removing the liner, pay careful attention to how it was installed. This will make reinstallation easier.

Tips and problem solving:

If you encounter any problems with the device or develop any pressure points or discoloration, contact your practitioner.

Arlington Heights
617 E. Golf Road, Suite 108
Arlington Heights, IL 60005
847-437-3929

Bannockburn
2101 Waukegan Road,
Suite 104
Bannockburn, IL 60015
847-444-0690

Lincoln Park/Chicago
2551 N. Clark St., Suite 200
Chicago, IL 60614
773-472-3663

Rush/Chicago
1725 W. Harrison St.
Suite 220
Chicago, IL 60612
312-942-2011

UIC/Chicago
1740 W. Taylor St.
Room C100
Chicago, IL 60612
312-996-6450

Hickory Hills
8641 W. 95th St.
Hickory Hills, IL 60457
708-599-8336

Naperville
1551 Bond St., Suite 111
Naperville, IL 60563
630-637-4638

Oakbrook Terrace
1S376 Summit Ave., Ct. E
Oakbrook Terrace, IL 60181
630-424-0392

Oak Park
401 Harrison Street
Oak Park, IL 60304
708-383-2257

Schererville
6629 W. Lincoln Hwy.
(Rt. 30), Suite 1
PO Box 507
Schererville, IN 46375
219-864-9501